


INSTRUCTIONS #6A MINI Modified Safety Pin Splint Dynamic Coiled Spring.

Open strap. Place finger into splint with curved finger band on bottom and in front of D.I.P. joint. Align coiled spring with D.I.P. joint. Position pad on strap (hook and loop compatible), pass strap over top of finger, under lateral wire, and back on top of finger. Secure to loop. Adjust as needed. Evaluate fit, function and instruct patient on use.

Lateral wires and finger bands can be carefully reshaped to improve fit and function. Remove from patient to modify. Clean with mild soap and damp towel. Air dry completely before reapplying.

Immediately contact your health care professional if you are experiencing loss of sensation, swelling, skin irritations or have any questions or concerns.

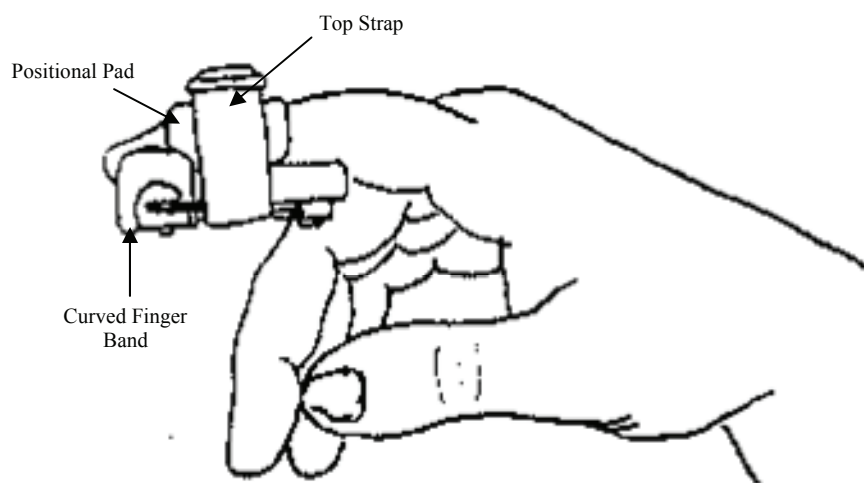

Bunnell #6A MINI Modified Safety Pin Splint to straighten D.I.P. joint

CAUTION: Federal Law restricts this device to sale by or on the order of a physician



Single patient use